

Nuovo kit salivare per il rilevamento dell'antigene Covid-19

96% Sensitività - 97% Specificità
NEWGENE2

NUOVO METODO DI CAMPIONAMENTO DELL'ESPETTORATO: PIÙ FACILE E SICURO DA ESEGUIRE, MAGGIORE PRECISIONE DEI RISULTATI, NON INVASIVO E NON FASTIDIOSO PER IL PAZIENTE

Il test dell'antigene serve a rilevare il virus stesso, quindi la selezione del campione è molto importante. Poiché l'espettorato è la secrezione dal tratto respiratorio dove i virus si raggruppano maggiormente, è relativamente più facile e accurato il rilevamento rispetto al campionamento nasale o nella gola.

A causa della distribuzione non uniforme del virus nella mucosa orofaringea, è molto probabile che durante il campionamento non venga assunto alcun virus o in piccolissima quantità e porti a risultati falsi negativi. Pertanto, l'affidabilità è inferiore a quella effettuata con l'espettorato.

La raccolta dell'espettorato può anche essere eseguita direttamente dal paziente nel pratico bicchierino in carta monouso fornito nel kit per ridurre il rischio di contagio per l'operatore rispetto all'esecuzione ravvicinata del tampone naso-gola.




Caratteristiche del prodotto

- 1 Nuovo rilevamento dell'antigene del coronavirus
- 2 Utilizza campioni di espettorato
- 3 Rilevamento veloce: risultato in 15 minuti
- 4 Alta precisione e facile da usare
- 5 Ogni kit contiene tutto il necessario per eseguire il test
- 6 Dispositivo IVD certificato CE registrato al Ministero della Salute


Componenti Scatola (25 pezzi)

- N° 25 • Kit di rilevamento
- N° 25 • Provetta per estrazione del campione
- N° 25 • Bastoncino con batuffolo di cotone
- N° 25 • Bicchierino di carta
- N° 01 • Foglietto illustrativo

15'

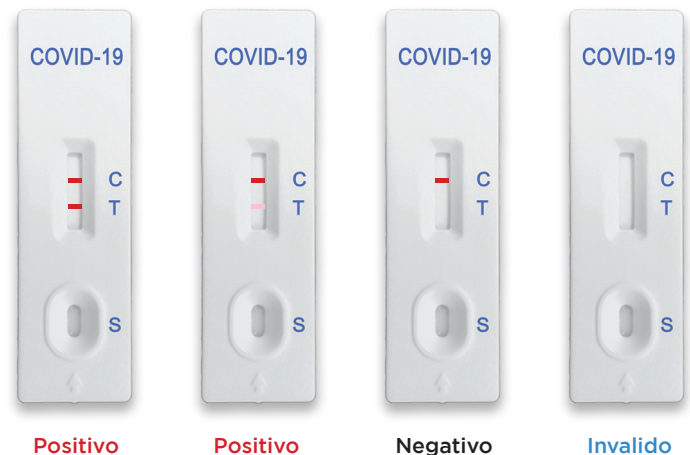

ESEMPIO UTILIZZO KIT:

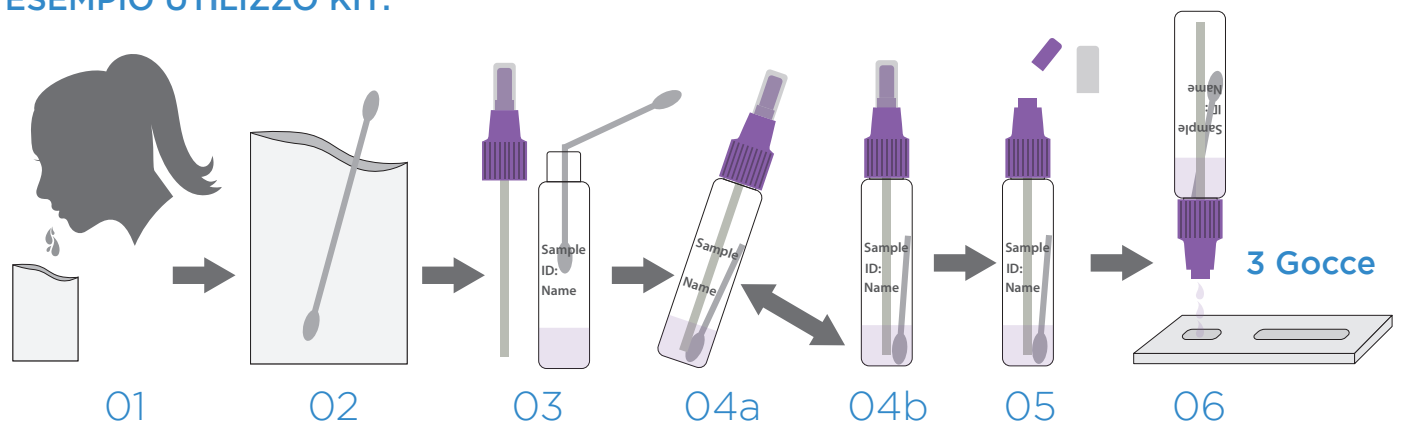

New salivary kit for the detection of the Covid-19 antigen

96% Sensitivity - 97% Specificity

NEWGENE2

NEW SPUTUM SAMPLING METHOD: EASIER TO DO, HIGHER ACCURACY, LESS INVASIVE OFFERS MORE COMFORT FOR THE PATIENT

Antigen test is to detect the virus itself, so sample selection is very important. Since sputum is the secretion from respiratory tract where viruses cluster the most, it is relatively easier and more accurate for detection versus the throat sampling. Because of the uneven distribution of the virus of the nasopharyngeal mucosa appearance, it is very likely that no virus or very small amount of virus is taken while sampling and lead to false negative result, when sampling via throat swab. Therefore, the accuracy will be lower than of saliva sampling (sputum).

The collection of sputum sample can be performed directly by the patient in the practical disposable paper cup supplied in the kit to reduce the risk of infection for the operator compared to the close execution of the nose-throat swab sampling.




Product features

1. New coronavirus antigen detection test
2. Use salivary samples
3. Fast detection: result in 15 minutes
4. High precision and easy to use
5. Each kit contains everything needed to perform the test
6. CE certified IVD device registered with the Ministry of Health

Box Components (25 pcs)

- N° 25 • Detection Kit
- N° 25 • Sample Extraction Tube
- N° 25 • Cotton Swab
- N° 25 • Paper Cup
- N° 01 • Package Insert

15'

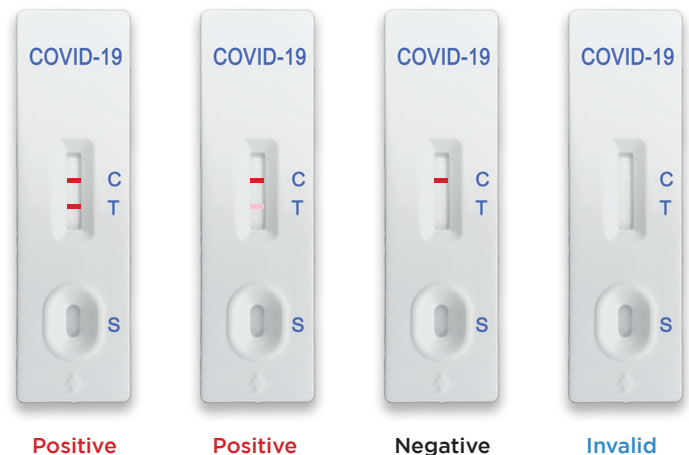

EXAMPLE OF KIT USE:

